



MESI ABPI MD: Cuff top tips


Make sure that the cuff makes good contact with the limb by following its anatomy to ensure accurate measurement. The cuff may not be completely straight, but this won't affect the measurement.

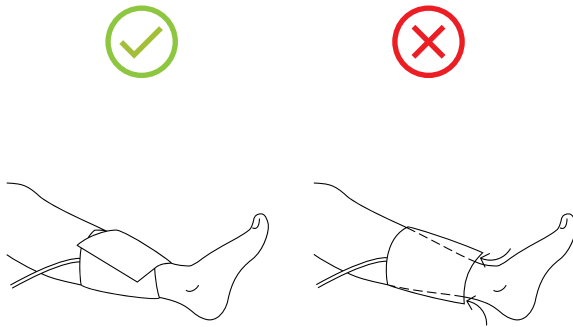

When putting the cuffs away, ensure they are folded flat and the bladders inside the cuffs are straightened. Do not roll the cuffs or leave them unfolded.

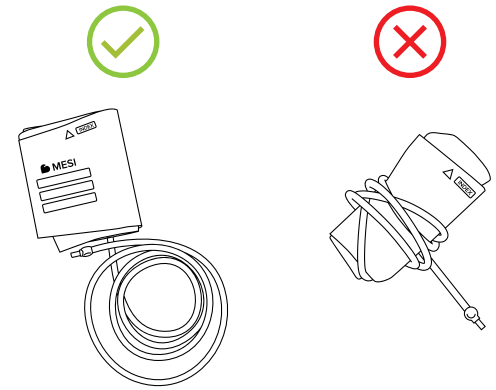

Ensure the correct cuff size is used for the limb by paying attention to the "OK" indicator. If the index on the cuff is outside the range, use a bigger cuff set.

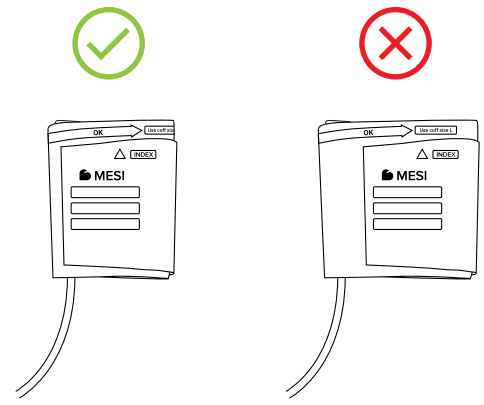

Make sure the tubes are straightened and not tucked under the limbs when performing the measurement.

